

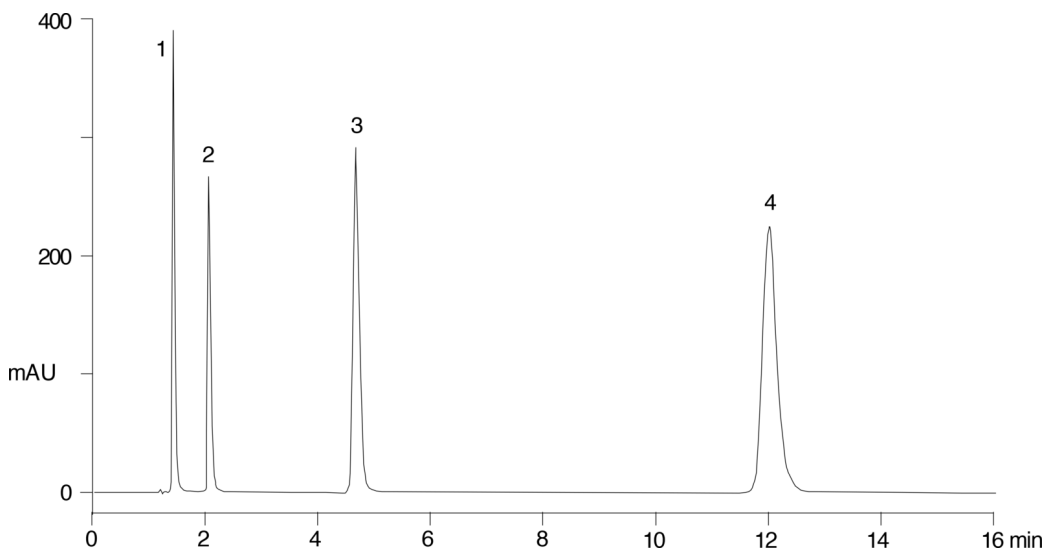
QC Test on Hyperclone 3u C18**Column:** HyperClone™ 3 µm ODS (C18) 120 Å, LC Column 100 x 4.6 mm, Ea**Dimensions:** 100 x 4.6 mm ID**Order No:** 00D-4356-E0**Elution Type:** Isocratic**Eluent A:** Water**Eluent B:** MeOH

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	30	70

Flow Rate: 1 mL/min**Col. Temp.:** ambient**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 254 nm (ambient)**Analyst Note:** SecurityGuard™ Guard Cartridge System extends column lifetime.

- SecurityGuard Cartridges, C18 4 x 3.0mm, 10/Pk Part No.: AJ0-4287

- Holder Part No.: KJ0-4282

**Products used in this application:****HyperClone™****ANALYTES:**

- 1 Benzamide
- 2 Acetophenone
- 3 Benzophenone
- 4 Biphenyl

