


USP 467 Procedure A - Class 1 by GC/FID on ZB-624**Column:** ZebtronTM ZB-624, GC Cap. Column 30 m x 0.32 mm x 1.80 μ m, Ea**Phase:** 6% Cyanopropylphenyl 94% Dimethylpolysiloxane**Dimensions:** 30 meters x 0.32 mm x 1.8 μ m**Order No:** 7HM-G005-31**Oven Profile:** 40 °C for 20 min to 240 °C @ 10 °C/min for 20 min**Carrier Gas:** Constant Flow Helium, 35 cm/sec**Injection:** Headspace 5:1 1 μ L @ 140°C**Detection:** Flame Ionization (FID) (250°C)**Analyst Note:** Sample Prepared as per USP Guidelines**Products used in this application:****ANALYTES:**

- 1 1,1-Dichloroethene
- 2 1,1,1-Trichloroethane
- 3 Carbon tetrachloride
- 4 Benzene
- 5 1,2-Dichloroethane

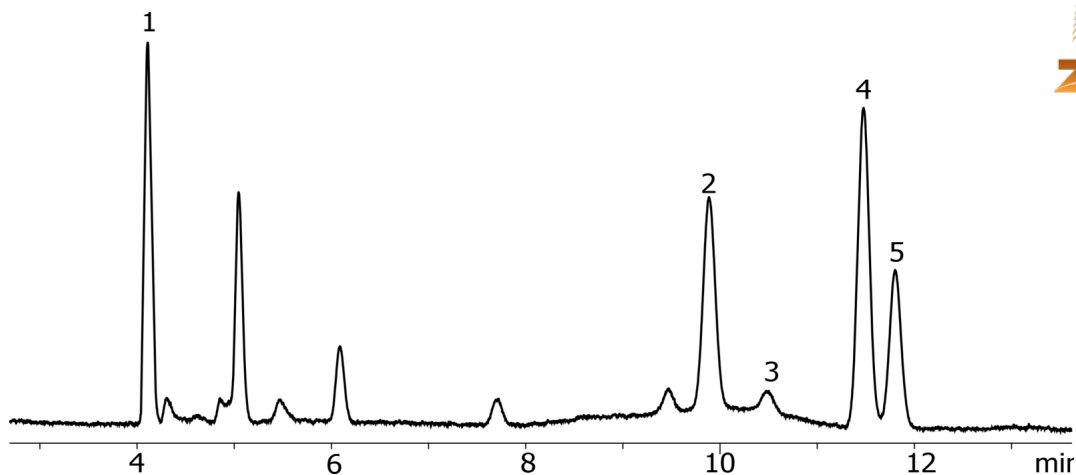