


**ASTM D6584: Calibration Standards for Biodiesel Analysis on ZB-35HT****Column:** Zebtron™ ZB-35HT, GC Cap. Column 15 m x 0.25 mm x 0.10 µm, Ea**Phase:** 35% Phenyl 65% Dimethylpolysiloxane**Dimensions:** 15 meters x 0.25 mm x 0.1 µm**Order No:** 7EG-G025-02**Oven Profile:****Carrier Gas:** Constant Flow Helium, 1.3 mL/min**Injection:** On-Column 0.000000000:1 0 µL @ 53°C**Detection:** Refractive Index (380°C)**Analyst Note:** A 3.0 m x 0.53 mm i.d. Guard Column was connected to the analytical column per ASTM method requirements.**Products used in this application:****ANALYTES:**

- 1 Glycerol
- 2 Butanetriol
- 3 1-Monooleoyl-rac-glycerol
- 4 Tricaprin
- 5 1,3-Diolein
- 6 Triolein

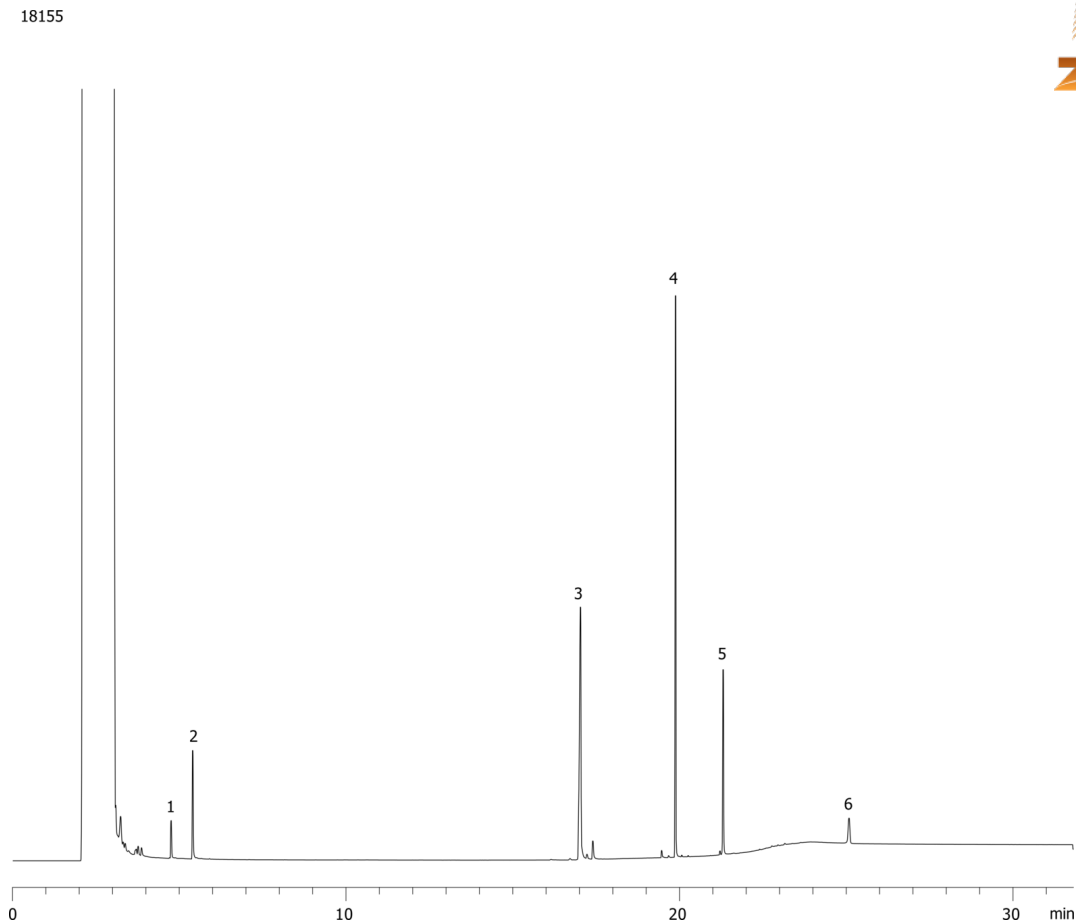