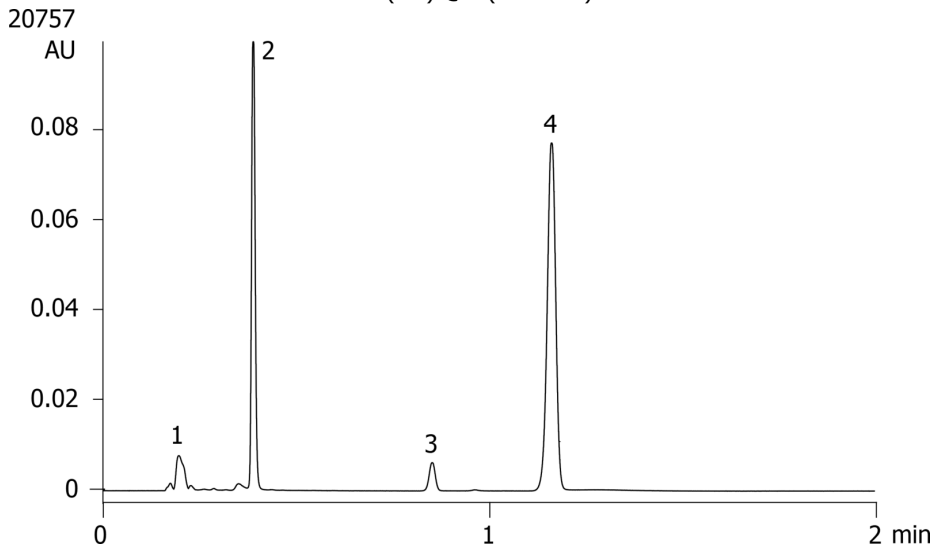


Prodigy Test Mix on Kinetex 1.7u C18 on Acquity System**Column:** Kinetex® 1.7 µm C18 100 Å, LC Column 50 x 2.1 mm, Ea**Dimensions:** 50 x 2.1 mm ID**Order No:** 00B-4475-AN**Elution Type:** Isocratic**Eluent A:** Water**Eluent B:** Acetonitrile

Gradient	Step No.	Time (min)	Pct A	Pct B
Profile:	1	0	50	50

Flow Rate: 0.5 mL/min**Col. Temp.:** 30 °C**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ (ambient)**ANALYTES:****1** Uracil

Retention Time: 0.203 min

2 Acetophenone

Retention Time: 0.395 min

3 Toluene

Retention Time: 0.857 min

4 Naphthalene

Retention Time: 1.165 min

**Products used in this application:**