

Nicotinic acid / Nicotinamide (1000 ng/mL) in Human Plasma by Impact on Gemini 3µm C18 100x4.6mm

Column: Gemini® 3 µm C18 110 Å, LC Column 100 x 4.6 mm, Ea

Dimensions: 100 x 4.6 mm ID

Order No: 00D-4439-E0

Elution Type: Gradient

Eluent A: 0.1% formic acid

Eluent B: Methanol 100%


Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	90	10
	2	2.5	10	90
	3	2.6	90	10
	4	4	90	10

Flow Rate: 0.6 mL/min

Col. Temp.: ambient

Detection: Electrospray Mass Spec (ESMS) @ (ambient)

Detector Info: <a target="_blank"

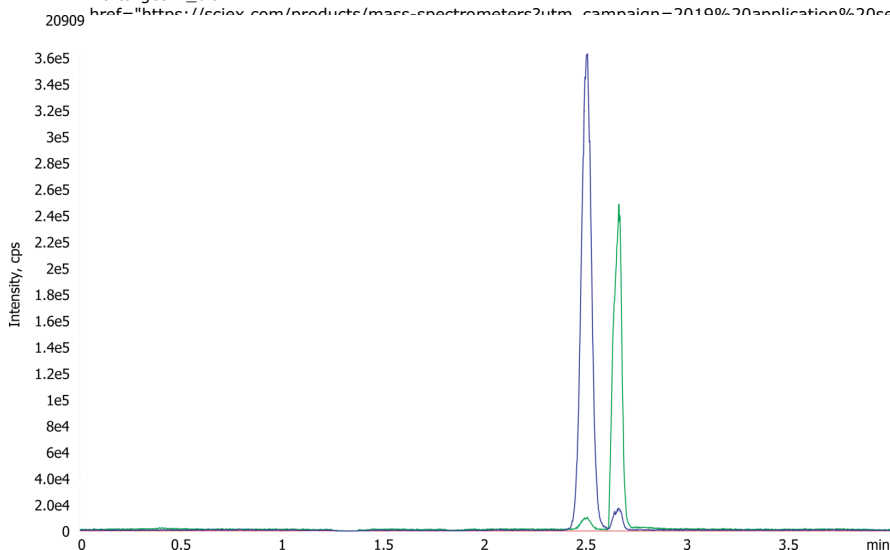

ANALYTES:

- 1 Nicotinamide**
Retention Time: 2.5 min
- 2 Nicotinic acid**
Retention Time: 2.66 min



Products used in this application:



Sample Preparation Details

for HPLC Application ID No.: 20909

Nicotinic acid / Nicotinamide (1000 ng/mL) in Human Plasma by Impact on Gemini 3µm C18 100x4.6mm

PRODUCT DESCRIPTION:

Impact™ Protein Precipitation, 2mL Square Well Filter Plate, 2/Pk

Order No.: CE0-7565

SOLID PHASE EXTRACTION (SPE) PROCEDURE:

Note: The solvent volumes shown below are for a Proprietary bed mass.

The solvent volumes will need to be adjusted for a smaller or larger bed mass.

Condition:

Load:

Wash:

Dry:

Elute:

Final Prep and Analysis:

Inject: 2 µL on HPLC Electrospray Mass Spec (ESMS) @ (ambient)

ANALYTES:		Spiked Conc. (ng/mL)	Log P	pKa	% Rec	%RSC (n=0)
1	Nicotinamide	1000			101	
2	Nicotinic acid	1000			96.1	

Note: This method is designed as a convenient starting point for further investigation and can be tailored to meet your extraction goals.
Call your local Phenomenex Representative for assistance in method development and optimization techniques.

©2025 Phenomenex Inc. All rights reserved.

For more information contact your Phenomenex Representative at support@phenomenex.com



Phenomenex products are available worldwide.

www.phenomenex.com

support@phenomenex.com