


EPA 539 using Kinetex 5u EVO C18 100x3.0mm**Column:** Kinetex® 5µm EVO C18 100 Å, LC Column 100 x 3.0 mm, Ea**Dimensions:** 100 x 3 mm ID**Order No:** 00D-4633-Y0**Elution Type:** Gradient**Eluent A:** 0.2% ammonium hydroxide**Eluent B:** Methanol with 0.2% ammonium hydroxide

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	65	35
	2	0.6	35	65
	3	7.5	35	65
	4	8.5	15	85
	5	13	15	85
	6	13.01	35	65
	7	15	35	65

Flow Rate: 0.3 mL/min**Col. Temp.:** 30 °C**Detection:** Electrospray Mass Spec (ESMS) @ (40 °C)**Detector Info:** SCIEX**ANALYTES:**

- 1 Estriol
Retention Time: 3.71 min
- 2 Equilin
Retention Time: 5.39 min
- 3 Estrone
Retention Time: 5.67 min
- 4 17-B-Estradiol
Retention Time: 5.84 min
- 5 17-a-Ethynylestradiol
Retention Time: 5.9 min
- 6 Androstenedione
Retention Time: 5.52 min
- 7 Testosterone
Retention Time: 6.13 min

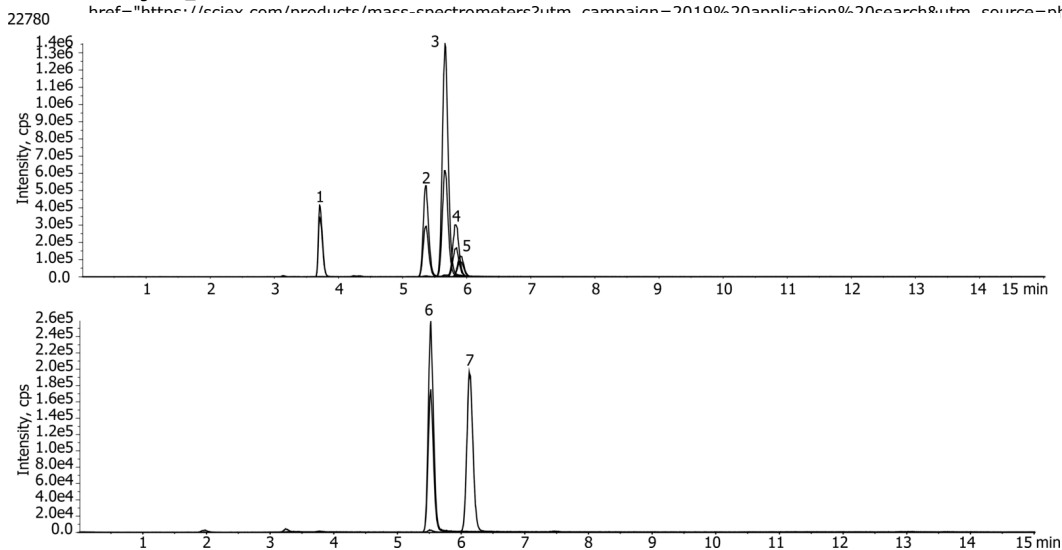