


Yarra 1.8 μ m SEC-X150 Batch-to-Batch Reproducibility**Column:** N/A**Dimensions:** N/A**Order No:** N/A**Elution Type:** N/A**Eluent A:** 0.1 M Sodium Phosphate, pH 6.8**Gradient** **Step No.** **Time (min)** **Pct A****Profile:** **1** 0 100**Flow Rate:** 0.3 mL/min**Col. Temp.:** ambient**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

23230

**ANALYTES:**

- 1** Thyroglobulin
- 2** IgA
- 3** IgG
- 4** Ovalbumin
- 5** Myoglobin
- 6** Uridine

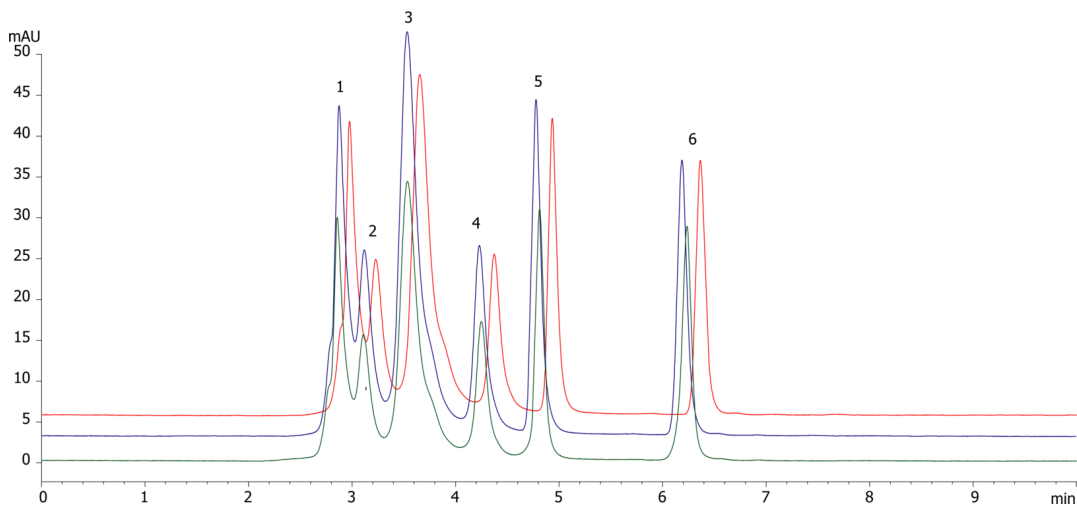