

FAMES In Rapeseed Oil by GC/FID on Zebron ZB-88

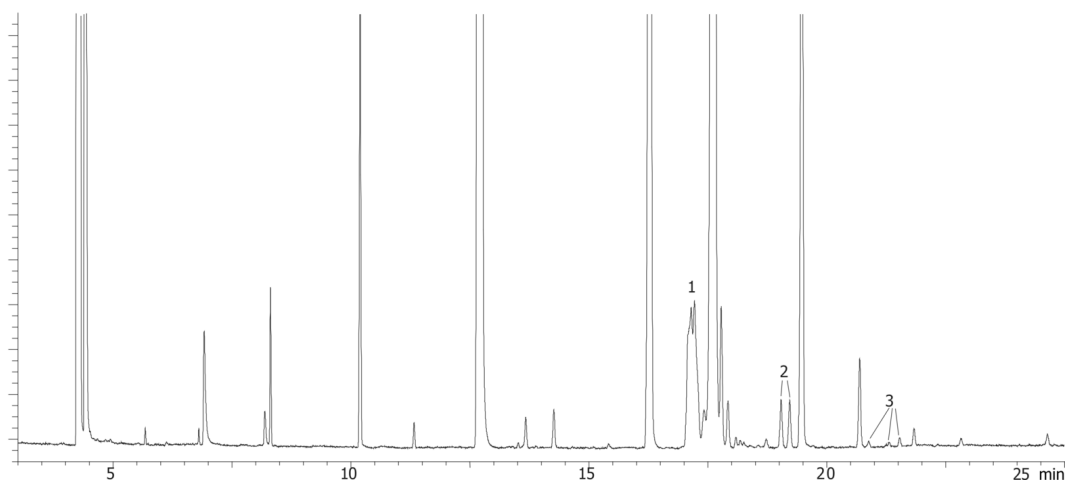
Column: N/A
Phase: N/A
Dimensions: N/A
Order No: N/A
Oven Profile: N/A

Carrier Gas: N/A
Injection: N/A
Detection: N/A

Analyst Note: Recommended Accessories:
Recommended Liner: Zebron PLUS Single Taper with Wool, 4 mm ID
Liner Part No.: AG2-0A13-05 (for Agilent systems)
Inlet Seal: AG0-8620 (Gold Plated Easy Seal)
Septum: AG0-4696 (PhenoRed-400)

Sample Preparation:
1. Weigh 100 mg of sample into 20 mL test tube
2. Add 10 mL of hexane
3. Add 100 μ L of 2N potassium hydroxide in methanol
4. Vortex for 30 seconds
5. Centrifuge and transfer upper layer into autosampler vial

23934

**ANALYTES:**

- 1** C18:1 trans
- 2** C18:2 trans
- 3** C18:3 trans

